


## Appendix N Residue Testing Flow Chart

Incoming tankers are screened for antibiotic residues by an approved Industry analyst/supervisor or by a Certified analyst/supervisor.

Daily monitoring performed on assays with a reader – checks must be valid before proceeding.  
Positive and negative control reactions are valid for the assay being used.

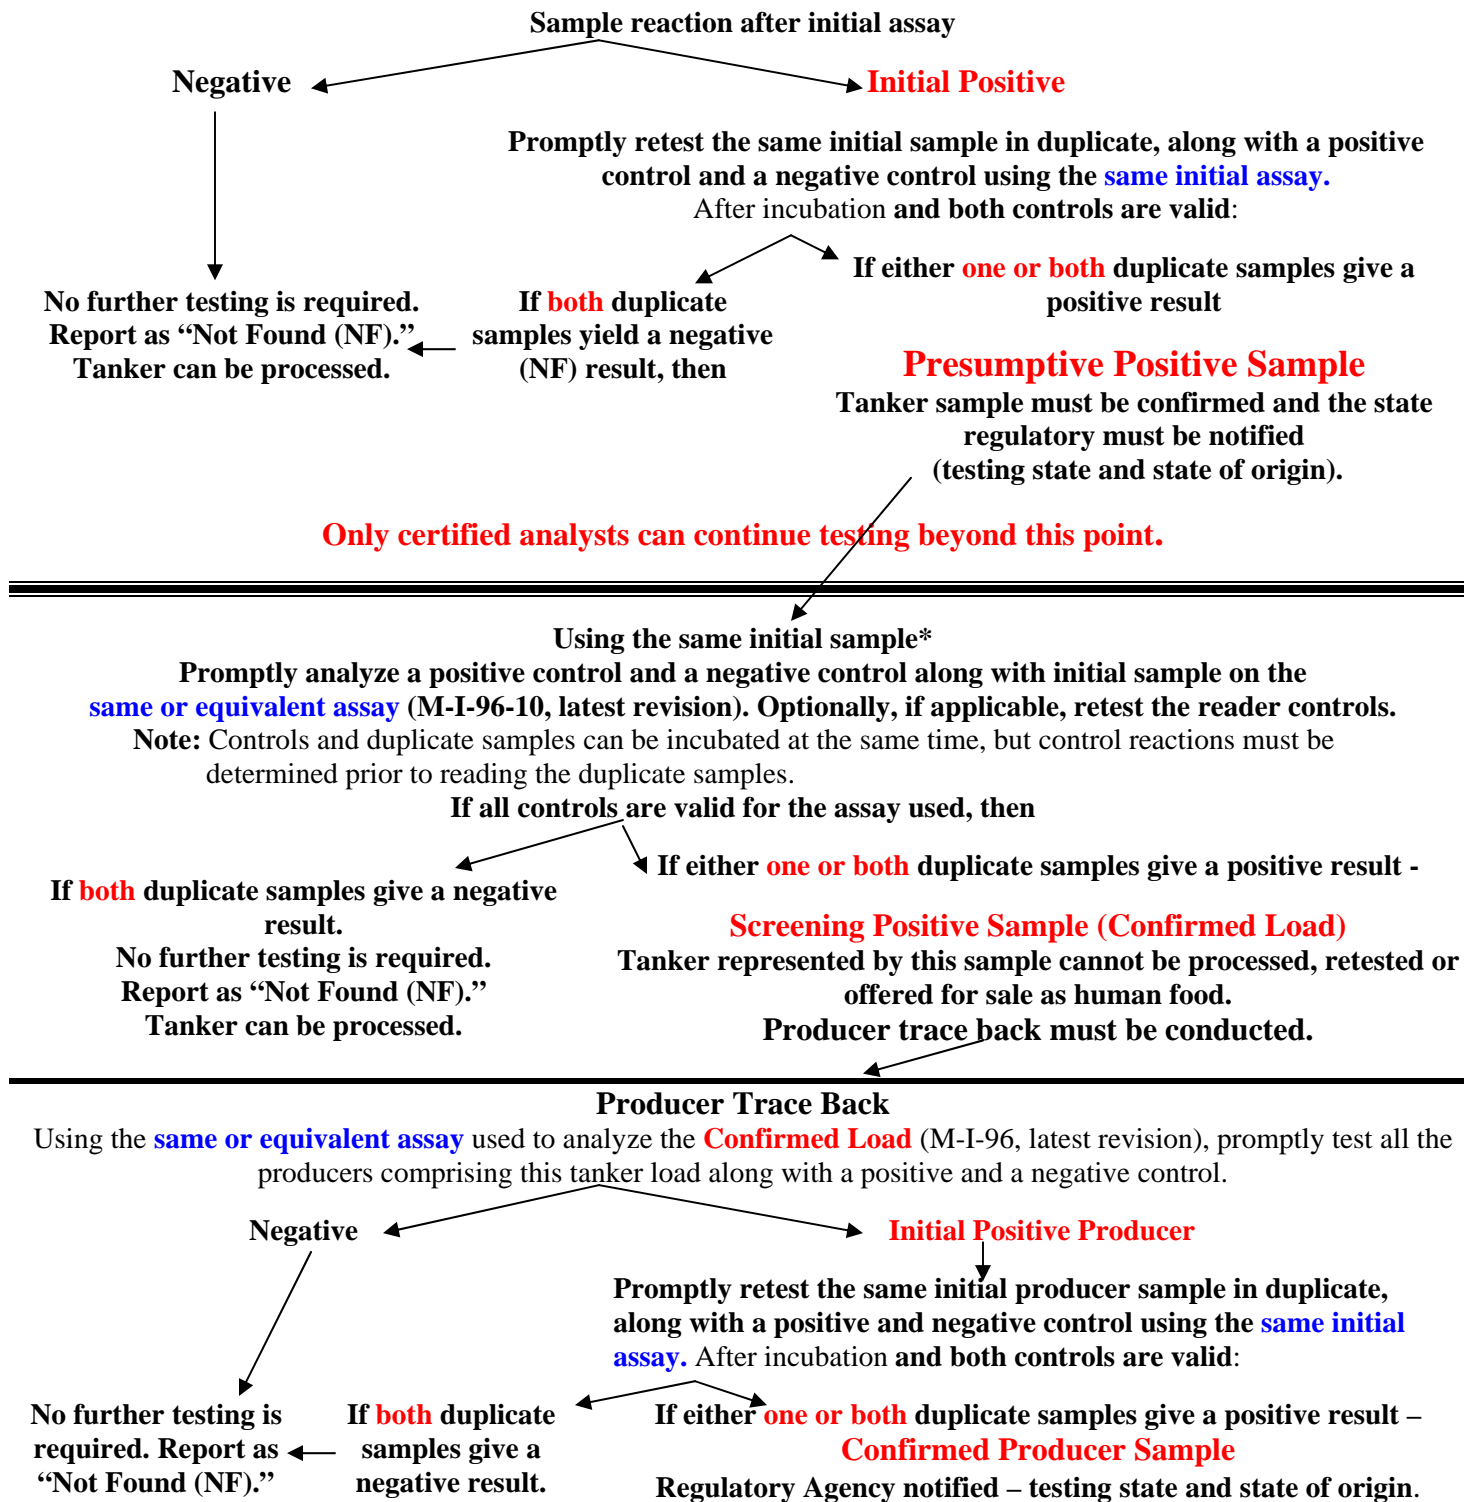

\*Presumptive Positive tanker can be re-sampled with the permission of the state regulatory agency prior to load confirmation. Records must indicate the reason(s) for re-sampling the tanker and the regulator contacted.